

final super-resolved image is reconstructed. The completely synthetic nature of the final image makes traditional analysis metrics such as the modulation transfer function ineffective. In fact, metrics for quantities as basic as spatial resolution have only recently been defined for localization microscopy⁹.

We are currently organizing the second edition of the challenge and the 2016 version will focus on 3D localization microscopy. While nanoscale-resolution 3D imaging is a powerful tool for studying protein ultrastructure *in vivo*, it also places significant extra demands on the image analysis.

3D localization microscopy works in a similar way to its 2D counterpart, but with the additional demand of encoding the axial position of a molecule in the shape of the point spread function. This extra requirement to estimate point spread function shape makes designing effective 3D algorithms much more challenging, particularly for low signal-to-noise data. Because of this, and probably because commercial 3D localization microscopy systems were less common until recently, 3D software has seen less development and characterization

than its 2D cousin. We hope to remedy this by robust testing of existing algorithms, and by creating a series of openly available simulated datasets to support future development. We are particularly keen to see how different 3D software performs away from optimal focus, since this is crucial to the effective depth of field of the technique.

At the same time we will continue the previous 2D challenge, updating it with new datasets to reflect the evolving demands of the field. It will be interesting to see how new challengers fare against the previous crop.

We hope that the provision of openly available experimentally realistic test datasets will also encourage participation of the broader image processing community. Advances have previously come from other disciplines as diverse as astronomy and compressed sensing. Who knows where the next one will come from?

The 2016 Single Molecule Localization Microscopy Challenge will run from April to June, with the results to be presented at the 6th Single Molecule Localization Microscopy Symposium, which is on 28–30 August

at the EPFL, Lausanne, Switzerland (<http://smlms.epfl.ch>). Further details and registration information can be found on the challenge website (<http://bigwww.epfl.ch/smlm/challenge2016>). Broad participation is warmly encouraged. □

Seamus Holden is at the Centre for Bacterial Cell Biology, Institute for Cell and Molecular Biosciences, Newcastle University, Newcastle Upon Tyne NE2 4AX, UK. Daniel Sage is in the Biomedical Imaging Group, School of Engineering, Ecole Polytechnique Fédérale de Lausanne, CH-1015 Lausanne, Switzerland.

e-mail: seamus.holden@ncl.ac.uk;

daniel.sage@epfl.ch

References

1. Betzig, E. *Science* **313**, 1642–1645 (2006).
2. Rust, M. J., Bates, M. & Zhuang, X. *Nature Methods* **3**, 793–795 (2006).
3. Holden, S. J., Uphoff, S. & Kapanidis, A. N. *Nature Methods* **8**, 279–280 (2011).
4. Huang, F., Schwartz, S. L., Byars, J. M. & Lidke, K. A. *Biomed. Opt. Express* **2**, 1377–1393 (2011).
5. Huang, F. *et al.* *Nature Methods* **10**, 653–658 (2013).
6. Wolter, S. *et al.* *Nature Methods* **9**, 1040–1041 (2012).
7. Smith, C. S., Joseph, N., Rieger, B. & Lidke, K. A. *Nature Methods* **7**, 373–375 (2010).
8. Sage, D. *et al.* *Nature Methods* **12**, 717–724 (2015).
9. Nieuwenhuizen, R. P. J. *et al.* *Nature Methods* **10**, 557–562 (2013).


PLASMONICS

Tunable spectrometer

A miniature mid-infrared spectrometer that combines the advantages of actuated microelectromechanical systems (MEMS) with the sensitivity of plasmonics has been built by scientists from Boston University (*ACS Photon.* **3**, 14–19; 2016). The device, a few hundred micrometres long and wide, consists of a gold film featuring a subwavelength hole array that is suspended above a gold reflector by an actuated polysilicon frame. Electrostatic actuation of the frame changes the gap between the gold film and the reflector, thus modifying the optical path length and the spectral response of the Fabry–Perot interferometer that they form.

“The additional mechanical degree of freedom provided by the MEMS will enable dynamic tuning of the spectral response of the system, making this device a powerful tool for differential measurements and spectrometry,” commented Thomas Stark from Boston University.

In recent years, subwavelength-sized holes in metal films have proved to be useful in various sensing applications due to their ability to greatly enhance the

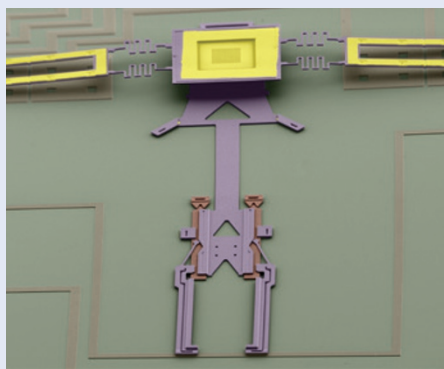

AMERICAN CHEMICAL SOCIETY

strength of the local electromagnetic field via the excitation of surface plasmons. This plasmonic enhancement can dramatically boost the sensitivity of absorption and Raman spectroscopy, allowing the techniques to reach new regimes of operation. However, the broad spectral width of a plasmon resonance means that it can be difficult to distinguish between closely spaced spectral absorption features.

In the Boston team's MEMS device (pictured), a polysilicon frame supported

a suspended gold film, in which an array of rectangular holes was fabricated using focused ion beam milling. The polysilicon frame was suspended 21.67 μm above the gold reflector. The size of the rectangular holes and the thickness of the gold film were 1,200 nm \times 500 nm and 100 nm, respectively. The team says that the suspended design has two advantages. First, surrounding the nanoscale holes with a homogeneous dielectric background provides higher quality plasmonic resonances. Second, the use of the polysilicon frame prevents the suspended gold film from being strained during the actuation of the MEMS device.

By tuning the distance between the gold film and the reflector from 1.7 μm to 21.67 μm , the spectral response of the MEMS device was modulated. Combining this modulation with phase-sensitive detection methods makes it possible to enhance the device's signal-to-noise ratio.

NORIAKI HORIUCHI