

SCIENTIFIC REPORTS



OPEN

Ratiometric and colorimetric near-infrared sensors for multi-channel detection of cyanide ion and their application to measure β -glucosidase

Panfei Xing¹, Yongqian Xu¹, Hongjuan Li¹, Shuhui Liu¹, Aiping Lu² & Shiguo Sun¹

A near-infrared sensor for cyanide ion (CN^-) was developed via internal charge transfer (ICT). This sensor can selectively detect CN^- either through dual-ratiometric fluorescence (logarithm of I_{414}/I_{564} and I_{803}/I_{564}) or under various absorption (356 and 440 nm) and emission (414, 564 and 803 nm) channels. Especially, the proposed method can be employed to measure β -glucosidase by detecting CN^- traces in commercial amygdalin samples.

Cyanide is an important raw material of pharmaceuticals, insecticides and fertilisers, as well as an indispensable reagent in metallurgy and gilded industry^{1,2}. However, CN^- can bind into mitochondrial cytochrome oxidase and inhibit critical enzymatic cascades in organisms, thus, CN^- is extremely detrimental. Consequent intracellular hypoxia often leads to central nervous system disorders, cardiovascular impairment or even death by suffocation within seconds to minutes³. It should be noted that CN^- can be derived from a variety of sources such as those from industrial accidents, pharmaceuticals, fire smoke and even some common foods⁴. For example, ingested amygdalin, which is one of the most typical cyanogenic glycosides found in kernels such as peach, apricot, cherry and almond, would be hydrolysed by the widely distributed natural β -glucosidase and generated hydrogen cyanide (HCN) in living organisms, leading to disruption of normal physiological activities and may result in death caused by rapid suffocation⁵. Therefore, CN^- monitoring has attracted much attention, and many techniques such as voltammetry, titrimetry, electrochemical and chromatography have been developed^{6–10}. Unfortunately, most of these methods require expensive equipment and are complicated for real-time analyses.

Recently, fluorometric detection has been increasingly used because of its low cost and rapid operation. In 2005, Geddes *et al.* reported a set of sensors for CN^- detection based on complexation between boronic acid and CN^- ¹¹. In 2008, Qin *et al.* described a reversible probe for CN^- based on the conversion of zinc ions in the presence of Cu^{2+} and CN^- ¹². On the basis of nucleophilic attack of the hydrogen-bonded carbonyl groups, Lee *et al.* developed a new method to detect CN^- in 2009¹³. In 2011, Lee *et al.* selectively detected CN^- based on the addition reaction between indole moiety and CN^- ¹⁴. With a similar mechanism, Shiraishi *et al.* recently synthesised a new fluorescent probe to selectively and sensitively detect CN^- ¹⁵. Most of these probes are designed on ON-OFF and OFF-ON mechanisms^{16–21}, wherein detection depends only on the changes in single emission and might be affected by external factors including excitation power, detector sensitivity and environment²².

According to literature^{14,15,23}, CN^- can conjugate with fluorescent dyes to modulate the ICT state and also elicit selective fluorescence changes. Thus, a novel fluorometric sensor SY (Fig. 1) was designed.

¹College of Science, Northwest A&F University, Yangling, Shaanxi, 712100, China. ²School of Chinese Medicine, Hong Kong Baptist University, Kowloon Tong, Hong Kong, 999077, China. Correspondence and requests for materials should be addressed to S.S. (email: sunsg@nwsuaf.edu.cn)

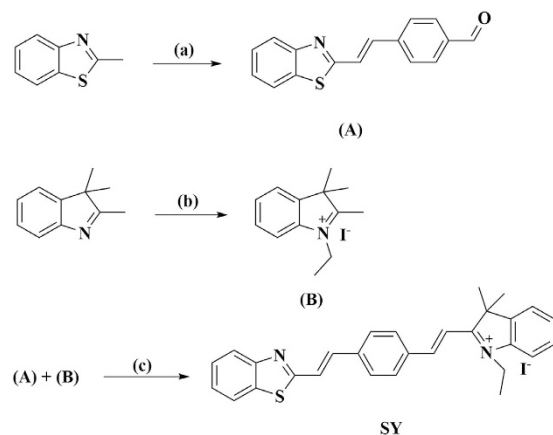


Figure 1. The synthesis of SY. Reagents and conditions: (a) 1,4-phthalaldehyde, acetic anhydride, acetic acid, 120°C, 6 h; (b) ethyl iodide, CH₃CN, reflux, 24 h; (c) acetic anhydride, CH₂Cl₂, anhydrous sodium acetate, stirring, 10 h.

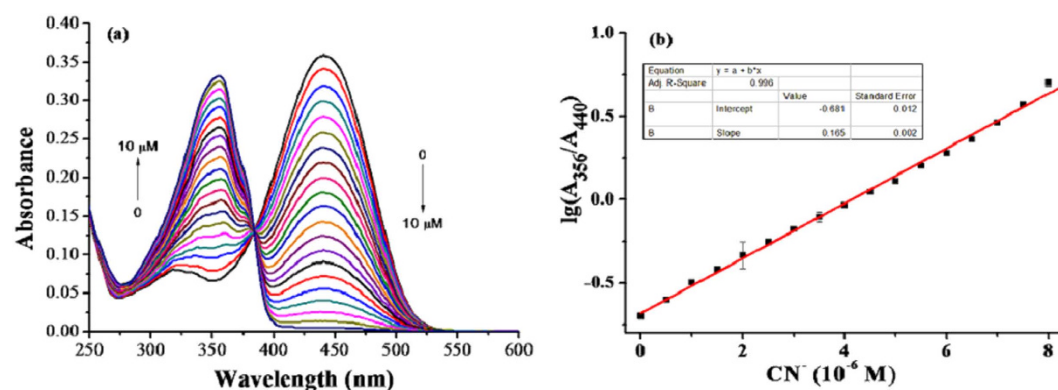


Figure 2. (a) UV-vis absorption titration spectra of SY (5 μM) in the presence of CN⁻ (0–10 μM) in acetonitrile at room temperature; **(b)** The linear relationship between the logarithm of the absorbance values (A_{356}/A_{440}) and CN⁻ concentration (0–10 μM).

SY displays an instantaneous (<5 s) fluorescence signal change in the presence of CN⁻ (0–10 μM) in acetonitrile, and a unique dual-ratiometric fluorescence (I_{414}/I_{564} and I_{803}/I_{564}) can be achieved for more accurate detection, especially that CN⁻ can be measured through multi-channels (under two absorption wavelengths of 356, 440 nm and three emission wavelengths of 414, 564, 803 nm), offering versatility during measurement. The applicability of SY was verified by its successful application in measuring β-glucosidase based on the above-mentioned typical hydrolysing ability towards amygdalin, which is useful in monitoring β-glucosidase level in living organisms because abnormal changes in β-glucosidase are linked to Gaucher's disease, Parkinson disease, pulmonary hypertension and even central nervous system disorders^{24,25}.

Results

UV-vis absorption titration spectra of SY upon addition of CN⁻. Firstly, the reaction time between SY and CN⁻ was tested. As shown in Fig. S1 (ESI[†]), SY can complete the reaction with CN⁻ within 5 s, indicating a rapid response of SY to CN⁻, which is beneficial in real-time detection. The UV-vis absorption titration spectra of SY (5 μM) were measured in acetonitrile at room temperature. As shown in Fig. 2a, the absorbance at 440 nm gradually decreased with the addition of CN⁻ and a new peak at 356 nm appeared, indicating that a chemical reaction occurred between CN⁻ and the indole group of SY. A colour change from yellow to colourless was dependent on CN⁻ concentration (Fig. S6), and 10 μM CN⁻ led to saturation. The logarithm of the absorbance ratio (A_{356}/A_{440}) produced a linear relationship ($R^2 = 0.996$) with CN⁻ concentration ranging from 0 μM to 7.5 μM (Fig. 2b), and the detection limit for CN⁻ based on $3\sigma/\text{slope}$ was $9.1 \times 10^{-8} \text{ M}$ ²⁶. In addition, the absorption values at each single peak also showed excellent linear relationship with $R^2 = 0.998$ (356 nm, 0–10 μM CN⁻) and $R^2 = 0.996$ (440 nm, 0–10 μM CN⁻) respectively (Fig. S2). The detection limit was $5.8 \times 10^{-7} \text{ M}$ at 356 nm and $3.9 \times 10^{-7} \text{ M}$ at 440 nm under similar condition.

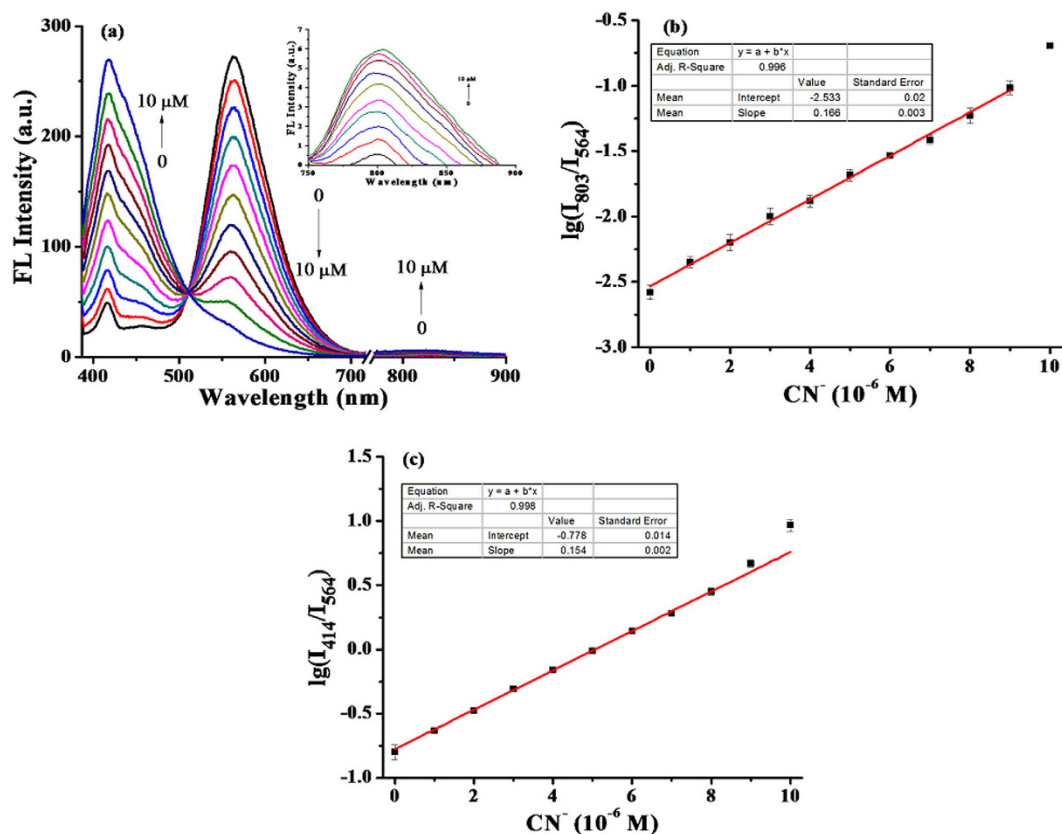


Figure 3. The fluorescence titration studies of SY towards CN^- . (a) Fluorescence spectra of SY ($5 \mu\text{M}$) upon addition of CN^- (0 – $10 \mu\text{M}$) at room temperature. Inset: enlarged fluorescence spectra from 750 nm to 900 nm , $\lambda_{\text{ex}} = 360 \text{ nm}$. (b) The corresponding linear relationship between the logarithm of the fluorescence ratio (I_{803}/I_{564}) in the presence of CN^- (0 – $9 \mu\text{M}$). (c) The corresponding linear relationship between the logarithm of the fluorescence ratio (I_{414}/I_{564}) in the presence of CN^- (0 – $10 \mu\text{M}$).

Fluorescence titration studies of SY upon addition of CN^- . Secondly, fluorescence titration studies on SY ($5 \mu\text{M}$) towards CN^- (0 – $10 \mu\text{M}$) were also performed, and a trend similar to that in UV-vis absorption titration was observed. With the addition of CN^- , the peak at 564 nm gradually decreased, and a new emission peak at 414 nm was recorded. It's worth noting that a concentration-dependent emission at 803 nm gradually and evidently increased owing to the nucleophilic attack of CN^- , which destroyed the conjugation of SY and blocked the ICT (Fig. 3a, Fig. S9–14)²⁷. Accordingly, an excellent linear relationship ($R^2 = 0.996$) was fitted between the logarithm of the fluorescence ratio (I_{803}/I_{564}) and CN^- concentration from $0 \mu\text{M}$ to $9 \mu\text{M}$ (Fig. 3b). The detection limit ($3\sigma/\text{slope}$) for CN^- was $7.3 \times 10^{-8} \text{ M}$ ²⁸. A second linear relationship ($R^2 = 0.998$) was also obtained between the logarithm of the fluorescence ratio (I_{414}/I_{564}) and CN^- concentration ranging from $0 \mu\text{M}$ to $10 \mu\text{M}$ at a detection limit of $5.4 \times 10^{-8} \text{ M}$ (Fig. 3c). As shown in Fig. S3 and S4, SY exhibited a good corresponding linear relationship with CN^- under each of the following emission channels: $R^2 = 0.998$ (414 nm , 0 – $10 \mu\text{M}$ CN^-), 0.998 (564 nm , 0 – $10 \mu\text{M}$ CN^-) and 0.995 (803 nm , 0 – $10 \mu\text{M}$ CN^-). The SY performance was subsequently studied in a mixing solvent of acetonitrile and increasing amount of water (0 – 20% , V/V, Fig. S5). Overall, the results verified the stability of SY.

Competitive experiments for CN^- selectivity. Furthermore, S^{2-} , CO_3^{2-} , ACO^- , $\text{S}_2\text{O}_3^{2-}$, SO_4^{2-} , I^- , Br^- , Cl^- , H_2PO_4^- , F^- , SCN^- , NO_2^- , glutathione (GSH), homocysteine (Hcy) and cysteine (Cys) were selected as interference ions to evaluate the selectivity of SY^{15,22}. As shown in Fig. S7, with the addition of these various analytes ($25 \mu\text{M}$ for each), SY did not show any significant fluorescence changes at 414 and 803 nm . By contrast, the addition of only $5 \mu\text{M}$ CN^- enhanced fluorescence at 414 and 803 nm , indicating that SY can selectively detect CN^- .

Discussion

^1H NMR and MS were used to verify the mechanism of SY in CN^- detection. As shown in Fig. S15a, the protons of the benzene ring in SY exhibited an upfield shift upon addition of CN^- . Similar results were observed on the protons of methyl and methylene groups (Fig. S15b), indicating the function of

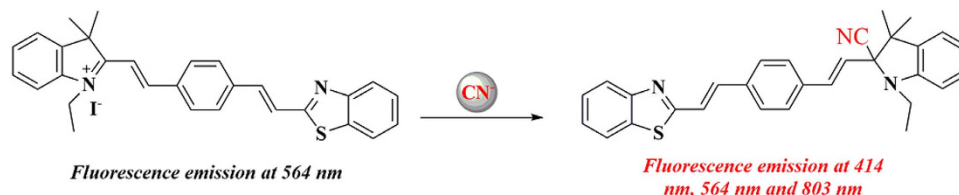


Figure 4. The mechanism of SY for CN^- .

samples	β -glucosidase (mU)	theoretical value (μM)	CN^- (I_{414}/I_{564} , μM)	RSD (I_{414}/I_{564} , %)	CN^- (I_{803}/I_{564} , μM)	RSD (I_{803}/I_{564} , %)
			1.0		1.0	
1	20	1.0	1.0	4.9	1.1	4.9
			1.1		1.0	
			5.2		5.3	
2	100	5.0	5.1	3.3	5.2	2.7
			5.2		5.3	
			7.4		7.6	
3	150	7.5	7.2	1.3	7.4	1.7
			7.6		7.3	

Table 1. β -Glucosidase assays in commercial amygdalin samples.

CN^- . The mass spectra (Fig. S24) further proved the SY-CN formation, m/z 462.36 (calc. = 462.20) corresponding to $[\text{SY} + \text{CN} + \text{H}]^+$.

Application for measuring enzyme activity *in vitro*. To confirm the applicability of the proposed method, SY was employed to study the activity of β -glucosidase by using cyanogenic glycoside amygdalin as indicator and SY as signal receptor²⁹. Moreover, β -Glucosidase catalysed the hydrolysis of amygdalin to free CN^- , initiating a signal change in the fluorescence spectrometer resulting from the reaction between SY and CN^- (Fig. 4). As shown in Table 1, the amount of CN^- detected by SY (the logarithm of the fluorescence ratio I_{414}/I_{564} , I_{803}/I_{564}) matched the concentrations of β -glucosidase. The relative standard deviations (RSDs) of I_{414}/I_{564} and I_{803}/I_{564} were lower than 4.9% and indicative of fine accuracy, further demonstrating the potential application of this method in CN^- determination. An alternative method (I_{414} , I_{564} and I_{803} , Table S1) was also provided to quantify CN^- . However, the RSDs of I_{414} , I_{564} and I_{803} were larger than those of I_{414}/I_{564} and I_{803}/I_{564} , indicating that enhanced precision can be achieved by ratiometric method.

In conclusion, a novel near-infrared probe SY for CN^- was successfully developed. SY exhibits a unique colorimetric in UV-vis and dual-ratiometric in fluorescence towards CN^- , resulting in more accurate detection. Moreover, its multi-channel detection offers versatility during measurement. The minimum detection limit of SY was 5.4×10^{-8} M. Furthermore, SY was successfully used to measure β -glucosidase. Overall, the results indicate that SY is a selective sensor for CN^- and a potential indicator of β -glucosidase.

Methods

Synthesis material and instruments. All solvents and chemical reagents were analytical grade and purchased from commercial suppliers. ^1H NMR and ^{13}C NMR spectra were recorded on a Bruker 500 AVANCE III spectrometer with chemical shifts reported in ppm at room temperature. Mass spectra were obtained with Thermo Fisher LCQ Fleet mass spectrometer (USA) and a LC/Q-ToF MS spectrometry (USA). Absorption spectra were collected by using a Shimadzu 1750 UV-visible spectrometer (Japan). Fluorescence spectra were measured with a Shimadzu RF-5301 fluorescence spectrometer (Japan) with both excitation and emission slits set at 10 nm if without further demonstration.

Compound (A) and (B) is prepared according to the reported literature^{30,31}.

Synthesis of (A) A mixture of 2-methylbenzimidazole (1.33 g, 5 mmol), p-phthaldialdehyde (1.34 g, 5 mmol) were added into 1.5 mL acetic anhydride and 1 mL acetic acid, stirring at 120°C for 6 h. Cooled to room temperature, 5 mL concentrated hydrochloric acid was added. Then 30% aqueous sodium hydroxide solution to make pH = 7, filtered and washed with water. The crude product was purified by column chromatography on silica gel using DCM to obtain a yellowish green crystal, 65% yield. ^1H

NMR (500 MHz, DMSO- d_6) δ 10.02 (s, 1 H), 8.11 (d, J = 6.6 Hz, 1 H), 8.00 (dd, J = 6.6, 2.3 Hz, 3 H), 7.94 (d, J = 6.6 Hz, 2 H), 7.78 (q, J = 13.2 Hz, 2 H), 7.58–7.49 (m, 1 H), 7.48–7.40 (m, 1 H).

Synthesis of **(B)** 2,3,3-trimethylindolenine (1 mL, 5.3 mmol) and iodoethane (0.9 mL, 10.6 mmol) were mixed in CH₃CN (15 mL), refluxing for 24 h. Cooled to room temperature, filtered, washed with ethyl acetate (3 × 10 mL) to obtain a pink crystal, 85% yield.

Synthesis of **SY A** mixture of **(A)** (0.5 mmol), **(B)** (0.5 mmol) and anhydrous sodium acetate (1 mmol) were added into 3 mL acetic anhydride, stirring at room temperature for 10 h. And then filtered, washed with water. The crude product was purified by column chromatography on silica gel using CH₂Cl₂ and ethyl acetate (1:1, V/V) to obtain a red solid, 60% yield. ¹H NMR (500 MHz, DMSO- d_6) δ 8.47 (d, J = 13.0 Hz, 1 H), 8.32 (d, J = 6.5 Hz, 2 H), 8.13 (d, J = 6.5 Hz, 1 H), 8.01 (t, J = 6.5 Hz, 3 H), 7.96 (dd, J = 4.9, 2.3 Hz, 1 H), 7.93–7.86 (m, 2 H), 7.77 (dd, J = 13.0, 2.0 Hz, 2 H), 7.64 (dd, J = 4.9, 2.3 Hz, 2 H), 7.57–7.50 (m, 1 H), 7.49–7.43 (m, 1 H), 4.76 (q, J = 5.7 Hz, 2 H), 1.84 (s, 6 H), 1.50 (t, J = 5.7 Hz, 3 H). ¹³C NMR (125 MHz, DMSO- d_6) δ 181.82, 166.49, 153.99, 153.30, 144.61, 140.91, 140.45, 136.55, 135.66, 134.83, 131.71, 130.11, 129.69, 128.86, 127.22, 126.29, 125.11, 123.66, 123.27, 122.83, 115.78, 113.37, 52.88, 42.89, 26.03, 14.38. HRMS: [M-I]⁺, calculated for [C₂₉H₂₇N₂S], 435.1889, found: 435.1887.

References

- Nguyen, H. H., Tran, T. & Wong, P. L. M. A kinetic study of the cementation of gold from cyanide solutions onto copper. *Hydrometallurgy* **46**, 55–69 (1997).
- Chaaban, M. A. Hazardous waste source reduction in materials and processing technologies. *J. Mater. Process. Technol.* **119**, 336–343 (2001).
- Hamel, J. A Review of Acute Cyanide Poisoning With a Treatment Update. *Crit. Care Nurse* **31**, 72–82 (2011).
- Baud, F. J. Cyanide: critical issues in diagnosis and treatment. *Hum. Exp. Toxicol.* **26**, 191–201 (2007).
- Rauws, A. G., Olling, M. & Timmerman, A. The pharmacokinetics of amygdalin. *Arch. Toxicol.* **49**, 311–319 (1982).
- Ding, G. *et al.* Electrofluorochromic Detection of Cyanide Anions Using a Nanoporous Polymer Electrode and the Detection Mechanism. *Chem. Eur. J.* **20**, 13226–13233 (2014).
- Xu, Z., Chen, X., Kim, H. N. & Yoon, J. Sensors for the optical detection of cyanide ion. *Chem. Soc. Rev.* **39**, 127–137 (2010).
- Breuer, P. L., Sutcliffe, C. A. & Meakin, R. L. Cyanide measurement by silver nitrate titration: Comparison of rhodanine and potentiometric end-points. *Hydrometallurgy* **106**, 135–140 (2011).
- Lou, B., Chen, Z. Q., Bian, Z. Q. & Huang, C. H. Multisignaling detection of cyanide anions based on an iridium(III) complex: remarkable enhancement of sensitivity by coordination effect. *New J. Chem.* **34**, 132–136 (2010).
- Mak, K. K. W., Yanase, H. & Renneberg, R. Cyanide fishing and cyanide detection in coral reef fish using chemical tests and biosensors. *Biosens. Bioelectron.* **20**, 2581–2593 (2005).
- Badugu, R., Lakowicz, J. R. & Geddes, C. D. Enhanced fluorescence cyanide detection at physiologically lethal levels: reduced ICT-based signal transduction. *J. Am. Chem. Soc.* **127**, 3635–3641 (2005).
- Lou, X., Zhang, L., Qin, J. & Li, Z. An alternative approach to develop a highly sensitive and selective chemosensor for the colorimetric sensing of cyanide in water. *Chem. Commun.* **44**, 5848–5850 (2008).
- Jo, J. & Lee, D. Turn-on fluorescence detection of cyanide in water: activation of latent fluorophores through remote hydrogen bonds that mimic peptide beta-turn motif. *J. Am. Chem. Soc.* **131**, 16283–16291 (2009).
- Kim, H. J., Ko, K. C., Lee, J. H., Lee, J. Y. & Kim, J. S. KCN sensor: unique chromogenic and ‘turn-on’ fluorescent chemodosimeter: rapid response and high selectivity. *Chem. Commun.* **47**, 2886–2888 (2011).
- Shiraishi, Y., Nakamura, M., Yamamoto, K. & Hirai, T. Rapid, selective, and sensitive fluorometric detection of cyanide anions in aqueous media by cyanine dyes with indolium-coumarin linkages. *Chem. Commun.* **50**, 11583–11586 (2014).
- Robbins, T. F., Qian, H., Su, X., Hughes, R. P. & Aprahamian, I. Cyanide Detection Using a Triazolopyridinium Salt. *Org. Lett.* **15**, 2386–2389 (2013).
- Chung, S. Y., Nam, S. W., Lim, J., Park, S. & Yoon, J. A highly selective cyanide sensing in water via fluorescence change and its application to *in vivo* imaging. *Chem. Commun.* **20**, 2866–2868 (2009).
- Jung, H. S., Han, J. H., Kim, Z. H., Kang, C. & Kim, J. S. Coumarin-Cu(II) Ensemble-Based Cyanide Sensing Chemodosimeter. *Org. Lett.* **13**, 5056–5059 (2011).
- Dong, M., Peng, Y., Dong, Y.-M., Tang, N. & Wang, Y.-W. A Selective, Colorimetric, and Fluorescent Chemodosimeter for Relay Recognition of Fluoride and Cyanide Anions Based on 1,1'-Binaphthyl Scaffold. *Org. Lett.* **14**, 130–133 (2011).
- Wang, P., Yao, Y. & Xue, M. A novel fluorescent probe for detecting paraquat and cyanide in water based on pillar[5]arene/10-methylacridinium iodide molecular recognition. *Chem. Commun.* **50**, 5064–5067 (2014).
- Chen, X. *et al.* A near-infrared fluorescent sensor for detection of cyanide in aqueous solution and its application for bioimaging. *Chem. Commun.* **46**, 8953–8955 (2010).
- Li, H., Wen, Z., Jin, L., Kan, Y. & Yin, B. A coumarin-Meldrum's acid conjugate based chemodosimetric probe for cyanide. *Chem. Commun.* **48**, 11659–11661 (2012).
- Lv, X. *et al.* Ratiometric fluorescence detection of cyanide based on a hybrid coumarin-hemicyanine dye: the large emission shift and the high selectivity. *Chem. Commun.* **47**, 12843–12845 (2011).
- Cullen, V. *et al.* Acid β -glucosidase mutants linked to gaucher disease, parkinson disease, and lewy body dementia alter α -synuclein processing. *Ann. Neurol.* **69**, 940–953 (2011).
- Lieberman, R. L. *et al.* Structure of acid β -glucosidase with pharmacological chaperone provides insight into Gaucher disease. *Nat. Chem. Biol.* **3**, 101–107 (2007).
- Sun, H. *et al.* A colorimetric lead (II) ions sensor based on selective recognition of G-quadruplexes by a clip-like cyanine dye. *Talanta* **136**, 210–214 (2015).
- Goswami, S., Paul, S. & Manna, A. Carbazole based hemicyanine dye for both “naked eye” and “NIR” fluorescence detection of CN⁻ in aqueous solution: from molecules to low cost devices (TLC plate sticks). *Dalton Trans.* **42**, 10682–10686 (2013).
- Xu, Y. *et al.* “ICT-not-quenching” near infrared ratiometric fluorescent detection of picric acid in aqueous media. *Chem. Commun.* **49**, 4764–4766 (2013).
- Jose, D. A., Elstner, M. & Schiller, A. Allosteric Indicator Displacement Enzyme Assay for a Cyanogenic Glycoside. *Chem. Eur. J.* **19**, 14451–14457 (2013).
- Kong, F. *et al.* A highly sensitive near-infrared fluorescent probe for cysteine and homocysteine in living cells. *Chem. Commun.* **49**, 9176–9178 (2013).
- Huang, Z. L. *et al.* Novel heterocycle-based organic molecules with two-photon induced blue fluorescent emission. *J. Mater. Chem.* **13**, 708–711 (2003).

Acknowledgements

This work was financially supported by the Scientific Research Foundation of Northwest A&F University (Z111021103 and Z111021107), the National Natural Science Foundation of China (No. 21206137, 21272030, 201205095 and 21476185), Shaanxi Province Science and Technology (No. 2013K12-03-23), State Key Laboratory of Chemo/Biosensing and Chemometrics, Hunan University (No. 2013005).

Author Contributions

S.G.S. supervised and interpreted the research. P.F.X. performed the measurements and wrote the manuscript. Y.Q.X., H.J.L., S.H.L. and A.P.L. helped with interpreted data and wrote the manuscript. All authors discussed the results and commented on the manuscript.

Additional Information

Supplementary information accompanies this paper at <http://www.nature.com/srep>

Competing financial interests: The authors declare there are no competing financial interests.

How to cite this article: Xing, P. *et al.* Ratiometric and colorimetric near-infrared sensors for multichannel detection of cyanide ion and their application to measure β -glucosidase. *Sci. Rep.* **5**, 16528; doi: 10.1038/srep16528 (2015).



This work is licensed under a Creative Commons Attribution 4.0 International License. The images or other third party material in this article are included in the article's Creative Commons license, unless indicated otherwise in the credit line; if the material is not included under the Creative Commons license, users will need to obtain permission from the license holder to reproduce the material. To view a copy of this license, visit <http://creativecommons.org/licenses/by/4.0/>