

SCIENTIFIC REPORTS



OPEN

Simple and effective exercise design for assessing *in vivo* mitochondrial function in clinical applications using ^{31}P magnetic resonance spectroscopy

Received: 24 September 2015

Accepted: 02 December 2015

Published: 11 January 2016

Alison Sleight^{1,2}, Victoria Lupson¹, Ajay Thankamony³, David B. Dunger³, David B. Savage⁴, T. Adrian Carpenter¹ & Graham J. Kemp⁵

The growing recognition of diseases associated with dysfunction of mitochondria poses an urgent need for simple measures of mitochondrial function. Assessment of the kinetics of replenishment of the phosphocreatine pool after exercise using ^{31}P magnetic resonance spectroscopy can provide an *in vivo* measure of mitochondrial function; however, the wider application of this technique appears limited by complex or expensive MR-compatible exercise equipment and protocols not easily tolerated by frail participants or those with reduced mental capacity. Here we describe a novel in-scanner exercise method which is patient-focused, inexpensive, remarkably simple and highly portable. The device exploits an MR-compatible high-density material (BaSO_4) to form a weight which is attached directly to the ankle, and a one-minute dynamic knee extension protocol produced highly reproducible measurements of post-exercise PCr recovery kinetics in both healthy subjects and patients. As sophisticated exercise equipment is unnecessary for this measurement, our extremely simple design provides an effective and easy-to-implement apparatus that is readily translatable across sites. Its design, being tailored to the needs of the patient, makes it particularly well suited to clinical applications, and we argue the potential of this method for investigating *in vivo* mitochondrial function in new cohorts of growing clinical interest.

Mitochondrial dysfunction is increasingly recognised as important in a variety of diseases including neurodegenerative, cardiovascular and metabolic disorders^{1–4}. ^{31}P magnetic resonance spectroscopy (^{31}P -MRS) has long been used to assess skeletal muscle mitochondrial function *in vivo* by measuring the kinetics of replenishment of the phosphocreatine (PCr) pool after exercise, which relates directly to oxidative ATP synthesis (reviewed extensively in⁵). The non-invasive nature of this technique permits multiple measurements in longitudinal intervention trials and arguably offers a more representative assessment of muscle mitochondrial function as it reflects the effects of an integrated cardiorespiratory/vascular system and permits a larger sample size than muscle biopsy. The growing recognition of the contribution of mitochondrion-associated diseases to the public health burden makes the use of this technique in clinical trials more important than ever.

A limitation to the wider application of the technique remains the need for MR-compatible exercise equipment suitable for use in clinical contexts. Commercial MR-compatible ergometers are increasingly available^{6–8}, but

¹Wolfson Brain Imaging Centre, University of Cambridge School of Clinical Medicine, Cambridge Biomedical Campus, Cambridge, CB2 0QQ, UK. ²National Institute for Health Research/Wellcome Trust Clinical Research Facility, Cambridge University Hospitals NHS Foundation Trust, Cambridge Biomedical Campus, Cambridge, CB2 0QQ, UK. ³Department of Paediatrics, University of Cambridge, Cambridge Biomedical Campus, Cambridge, CB2 0QQ, UK.

⁴University of Cambridge Metabolic Research Laboratories, Wellcome Trust-Medical Research Council Institute of Metabolic Science, Cambridge, CB2 0QQ, UK. ⁵Magnetic Resonance & Image Analysis Research Centre, Department of Musculoskeletal Biology and MRC – Arthritis Research UK Centre for Integrated research into Musculoskeletal Ageing, University of Liverpool, Liverpool, L69 3GE, UK. Correspondence and requests for materials should be addressed to A.S. (email: as626@wbic.cam.ac.uk)



Figure 1. Innovative MR-compatible high density material barium sulfate. Barium sulfate (BaSO_4) of mass 1 kg placed within a sealed freezer bag (shown next to a computer mouse for context).

these can be expensive and there is a long tradition of in-house construction of exercise equipment^{9–24}. Exercise may be static (isometric) or dynamic (isotonic); isometric exercise is conveniently scaled to maximum voluntary contraction *in situ*^{10,11,14,16–18,24}, but adjusting exercise intensity by interpreting force feedback^{10,13,14,16,18,23} can be challenging. Calibrated dynamic exercise typically requires complex resistance equipment^{7,11,16,17} or pulley systems to transfer the workload outside the bore^{15,19,20,22}, and in all systems participant posture is an important comfort consideration.

PCr recovery kinetics following exercise in which cell pH does not change much is well-known to be first-order, characterized by an exponential rate constant (k_{PCr}) that is independent of the degree of PCr depletion, and which is directly proportional to what may be physiologically regarded as functional mitochondrial capacity, generally insensitive to the details of the exercise perturbation⁵. Thus to assess muscle mitochondrial function needs only a way of producing moderate PCr depletion, which can be achieved by simple exercise methods rather than requiring sophisticated equipment. Here we exploit this and set out to design a simple, patient-friendly MR exercise method that is inexpensive and permits measurements of *in vivo* mitochondrial function easily in a clinical context where patients may have limited exercise tolerance and/or reduced mental capacity.

Methods

Participants. 26 (24 M, 2 F) participants with mean \pm SEM age 34.9 ± 1.7 y undertook ³¹P-MRS measurements on a Siemens MAGNETOM 3 T scanner. The participants consisted of one 30 y female control subject with a BMI of 21.3 kg/m^2 who undertook 2.5 minutes of exercise in a Siemens 3 T Trio scanner, one female 40 y lipodystrophic patient (BMI 20.3 kg/m^2) who performed the optimised exercise protocol in a Siemens 3 T Verio scanner, and 24 healthy non obese Caucasian male volunteers who underwent the optimised exercise protocol on two consecutive days in a Siemens 3 T Verio scanner.

Each participant provided written informed consent and all studies were conducted in accordance with the Declaration of Helsinki. Ethical approval was granted by Cambridgeshire 2 Research Ethics Committee, United Kingdom (for the control subject dataset shown), by the National Health Service Research Ethics Committee, United Kingdom (patient dataset shown), and by Cambridge Local Research Ethics Committee, United Kingdom (the 24 individuals who comprise the reproducibility statistics).

Workload methodology. This design exploits the high density of the MR-compatible material barium sulfate (BaSO_4), whose specific gravity is 4.5 (cf. 1.0 for water and 1.5 for dry sand²⁵). This permits enough mass (workload) to be placed within the scanner bore and circumvents the need for complex and/or expensive resistance equipment or pulley systems. Barium sulfate is relatively inexpensive and although pure BaSO_4 is MR-safe, any purchased BaSO_4 that might contain magnetically susceptible impurities should be tested. To permit an individual-specific workload, the barium sulfate was placed in sealable freezer bags (Fig. 1) following relevant safety data sheet advice, to form bags of differing weights (e.g. 1.00, 0.50, 0.20, 0.15, 0.10, 0.05 kg).

Exercise design. The participants were positioned in the comfortable feet-first supine position with their knees placed over a 14.5 cm diameter cylindrical foam and their feet placed in the resulting recess, as shown in Fig. 2. This configuration minimizes axial surface coil orientations and provides a wide angle of rotation for knee extension exercise. The appropriate mass (see Section ‘Ankle weight calculation’) was placed over the participant’s right ankle using a custom made dual-pocket ‘bag’ made from non-stretchable cord denim (Fig. 3A), with equal weights of BaSO_4 either side of the ankle. Figure 3B,C shows dimensions of the holder which can hold sufficient mass (up to ~ 9 kg), without the bag wrapping under the ankle. We found that the ankle weight did not move significantly relative to the leg during exercise.

Exercise MRS protocol. The exercise consisted of knee extensions of the right leg from the scanner table base to full knee extension, with the appropriate weight placed over the right ankle. This was performed at 0.5 Hz

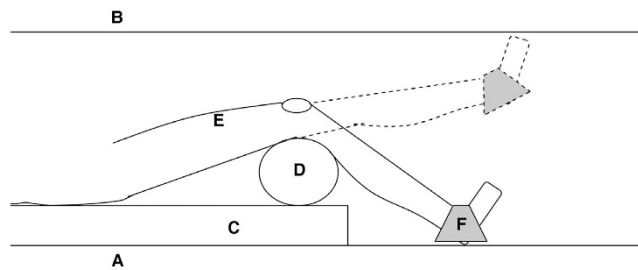


Figure 2. Schematic representation of the exercise design. Sagittal cross sectional profile through the scanner bore showing the exercise design *in situ*. The patient performs knee extension from the table base (A) to full knee extension (B), with a typical 45° angle of rotation resulting (Siemens MAGNETOM 3 T Verio). The body of the patient lies on the vendor's standard foam padding (C), displaced left such that their right leg is as near to isocentre as feasible. The posterior aspect of their knees rest over a firm cylindrical foam (D) of diameter 14.5 cm (standard Siemens equipment), with their ankle resting in the resulting recess in order to maximise exercise rotation. The coil is attached to the participant's quadriceps (E) over the muscle group of interest, and the MR-compatible weight and holder placed over the ankle (F).

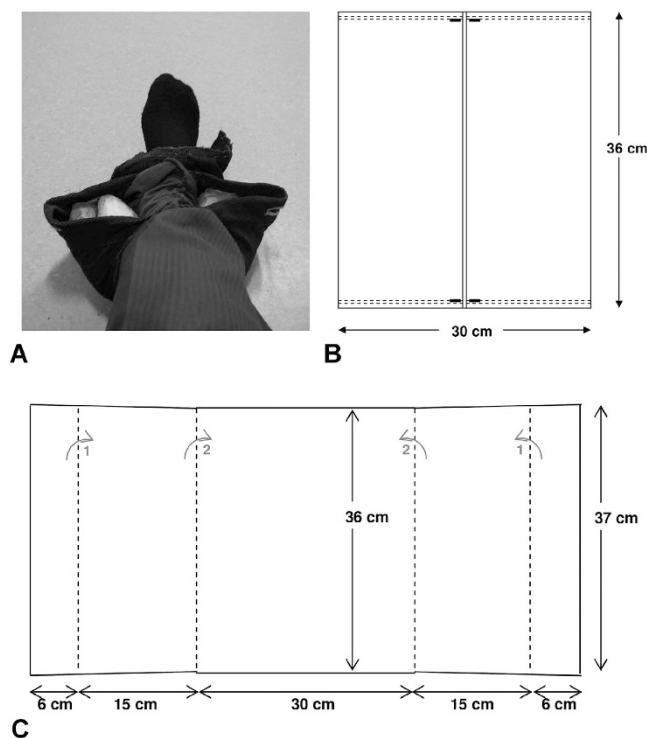


Figure 3. The dual-pocket ankle weight holder. The dual-pocket ankle weight holder filled with 3.0 kg (1.5 kg either side), placed over the ankle (A). Schematic representation illustrating dimensions of the built ankle weight holder when laid flat (B), and material prior to assembly (C). The dashed lines in (B) represent the location of strong machine stitching, and in (C) identify the material fold lines such that fold 1 (grey arrow), then fold 2 (grey arrow) are performed prior to stitching as denoted in (B). Fold 1 aids in ensuring the barium sulfate parcels remain in the holder with heavy workloads.

and gated such that, with subject compliance, the MR acquisition always occurred with the leg in the 'down' position. This was achieved using pre-recorded headphone instructions of up/down commands and warning of exercise onset and cessation. All participants were shown a training video prior to the scan to ensure they were familiar with the exercise protocol and undertook a brief practice before full entry to the scanner bore. One healthy female performed 2.5 minutes of this exercise and dynamic measurements of [PCr] and pH recorded (Fig. 4). From this an optimised exercise protocol was developed.

Ankle weight calculation. Volunteers' maximal voluntary contraction (MVC) was determined the previous day using a dynamometer chair set to knee extension from -45° to 0° , where 0° is knee extension without hyperextension (i.e. similar angles of exercise as in the scanner). Participants undertook an isokinetic protocol consisting of three knee extensions with gentle encouragement, and peak torque from their best repetition was

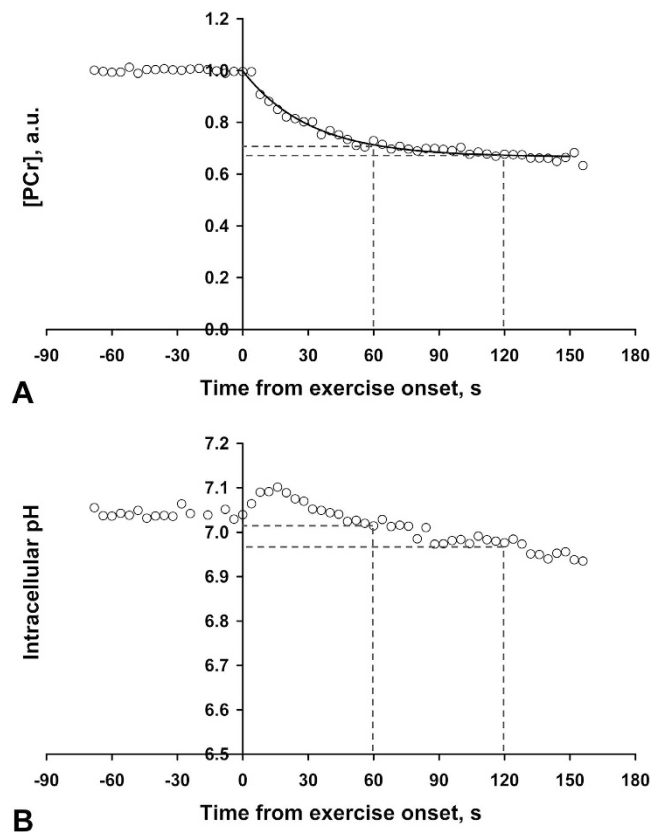


Figure 4. Phosphocreatine (PCr) and pH timecourse prior to and during exercise in an adult control. White circles represent [PCr] (A) and intracellular pH (B), as determined from individual spectra of ^{31}P -MRS data with a TR of 4s. Data acquired on a Siemens MAGNETOM 3T Trio (Erlangen, Germany) in a healthy adult volunteer performing exercise as outlined in Methods: Exercise MRS protocol, with a total ankle weight of 2.7 kg. The solid line in (A) represents a mono-exponential fit to the PCr exercise data. Dashed lines aid visualization as to the fractional PCr depletion (A) and intracellular pH (B), after both 1 and 2 minutes of exercise.

recorded as their MVC. Standardisation of PCr depletion between participants was achieved by altering the ankle weight to a fraction of their MVC such that $m = 0.131 \text{ MVC}/(\text{g}\cdot\text{L})$, where m is the ankle weight in kg, MVC the torque in Nm, g is 9.81 ms^{-2} , and L is the leg length in meters defined as the lateral femoral condyle to malleolus distance. In the study of 24 healthy non-obese male volunteers, who had height (mean \pm SEM) 180.5 ± 1.5 cm, leg length was not measured and L was assumed to be 42 cm, thereby providing $m = 0.0318 \text{ MVC}$. The target PCr depletion was 20–25% of basal [PCr] and more than 40% depletion was undesired.

^{31}P -MRS acquisition and analysis parameters. A 9 cm diameter ^{31}P (with butterfly-design ^1H) transmit-receive flex coil was used for all participants. Data acquisition and analysis methods were as in^{1,26}, but here data have been averaged to an effective time resolution of 8 s prior to PCr recovery fitting with a mono-exponential function (where the mean end-recovery PCr was calculated from the post exercise 8 s averaged time points 155–219 s inclusive). The intracellular pH was determined from the chemical shift of inorganic phosphate relative to PCr²⁷. The rate constant of post-exercise PCr resynthesis, k_{PCr} , was found using a two parameter mono-exponential fit as previously described²⁶, and is taken as a measure of muscle mitochondrial function⁵.

Reproducibility of the PCr recovery rate constant. The level of agreement in k_{PCr} repeatability (within a test session) and reproducibility (between test sessions) were assessed from a study of 24 individuals who underwent the optimised exercise protocol on two consecutive days as part of a fasting study (at 8 and 28 h of fasting)²⁸. Bland-Altman analysis was performed and the mean difference (bias) between the two measures was calculated then tested against zero using a one sample t-test. Individuals' CV of repeatability was assessed as the SD/mean of the two k_{PCr} values obtained at their Day-1 scan. The individuals' mean k_{PCr} for both Day-1 and Day-2 were then used for an estimate of CV of reproducibility with the fasting intervention of the study (which was found to have no significant effect overall on PCr recovery); this is therefore an upper limit on CV without any intervention.

Statistics. Statistical analysis was performed in IBM SPSS Statistics 21 (IBM Inc., Armonk, NY, USA), with significance set at $p < 0.05$. Quantitative data are presented as mean \pm SEM, unless otherwise stated.

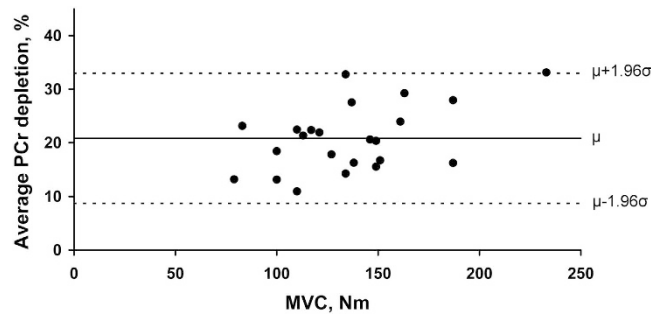


Figure 5. Percentage phosphocreatine (PCr) depletion after one minute of in-scanner exercise against participants' previously determined maximal voluntary contraction (MVC) in 23 healthy males. Black circles represent individuals' average PCr depletion on Day-1 (relative to basal levels) after performing one minute of exercise (optimised exercise protocol) with ankle weight as determined in Section 'Methods: Ankle weight calculation', against their MVC as assessed from the dynamometer chair. The solid line represents the mean PCr depletion (μ), and dashed lines the mean PCr depletion ± 1.96 SD.

Results

Exercise design. All participants found the exercise comfortable and completed the exercise protocol with no reported negative feedback. The Siemens standard 14.5 cm diameter foam cylinder placed under the volunteers' knee (Fig. 2) appeared to be appropriate for patient comfort whilst having enough solidity to minimise foam compression at the highest workloads.

We have implemented this exercise design in two MR scanners with differing bore dimensions (Siemens MAGNETOM 3 T Trio (Fig. 4) and 3 T Verio (Figs 5–7), Erlangen, Germany), demonstrating the ease of translating this method across MR scanner models.

Exercise MRS protocol. Figure 4A illustrates well controlled PCr depletion during this exercise, and demonstrates the exponential PCr decline expected during relatively low power exercise (as emphasised by dashed lines showing very little change from 1 to 2 minutes of exercise). Figure 4B shows the corresponding intracellular pH timecourse which reveals an insignificant pH change relative to basal after 1 minute, but a noticeable pH decrease after 2 minutes of exercise. Thus an exercise duration of 1 minute was chosen to minimise participant effort (which also incidentally aids compliance) and reduce the complicating effects of pH change on the interpretation of PCr recovery kinetics⁵. It is not necessary to establish a stable PCr before measurement of PCr recovery as the interpretation of k_{PCr} is independent of this⁵. In order to acquire two PCr recovery measurements which can then be averaged to improve precision, or allow two attempts at the measurement in patient groups who may be less tolerant or compliant of the exercise, the optimised protocol to measure *in vivo* mitochondrial function consisted of two 1 minute exercise durations (total scan 12 mins consisting of 1 min rest, 1 min exercise and 4 mins recovery, which is then all repeated).

Ankle weight calculation. One scan was lost due to hardware failure, leaving data from 23 individuals who underwent the optimised exercise protocol on Day-1 using an ankle weight calculated from their MVC (Methods section). Figure 5 illustrates the consistency of the percentage PCr depletion generated over the range of MVC's measured (79–233 Nm). Mean percentage PCr depletion relative to basal was $20.8 \pm 1.3\%$. Average PCr depletion significantly correlated with MVC (Pearson's $r = 0.482$, $p = 0.02$), though not when the possible outlier at high MVC was eliminated ($p = 0.16$).

Reproducibility of the PCr recovery constant. Three individuals did not undertake the ³¹P measurement on Day-2 and two ³¹P scans were lost due to hardware failure (one each day). 92% of all exercise bouts were participant compliant. The PCr linewidth was 6.6 ± 0.5 Hz on Day-1. Figure 6 shows Bland-Altman plots for test-retest analysis of k_{PCr} repeatability (Fig. 6A) and k_{PCr} reproducibility over the two days (Fig. 6B), in the 19 healthy individuals. There was no significant mean bias, nor proportional bias in either Fig. 6A,B. The mean CV of repeatability and reproducibility was $5.0 \pm 1.0\%$ and $8.2 \pm 1.5\%$ respectively. The mean PCr depletion of the Day-1 and Day-2 test sessions was $20.8 \pm 1.0\%$ and $19.2 \pm 1.5\%$ respectively. Figure 7A demonstrates the mean PCr timecourse from the 19 volunteers' Day-1 visit, and illustrates the consistency in mean PCr depletion at end of exercise bouts 1 and 2 ($20.0 \pm 1.3\%$ and $21.7 \pm 1.8\%$) respectively. Apparent slight increases in mean [PCr] at the start of exercise bout 1 and during exercise bout 2, may reflect incorrect exercise timing due to misinterpretation of the instructions in this cohort who did not have a prescan rehearsal to the timed instructions. This is not important when we only measure and fit the PCr kinetics of the resynthesis, and this method yielded highly consistent mean k_{PCr} values of $2.47 \pm 0.17 \text{ min}^{-1}$ and $2.44 \pm 0.15 \text{ min}^{-1}$ for post-exercise recovery 1 and 2 respectively.

Patient dataset. Figure 7B illustrates the PCr timecourse in a lipodystrophic patient performing the optimised exercise protocol for measurement of *in vivo* mitochondrial function. In this patient the ankle weight was 4.4 kg, which led to 30% and 33% PCr depletion at the end of exercise bouts 1 and 2 respectively. The k_{PCr} values

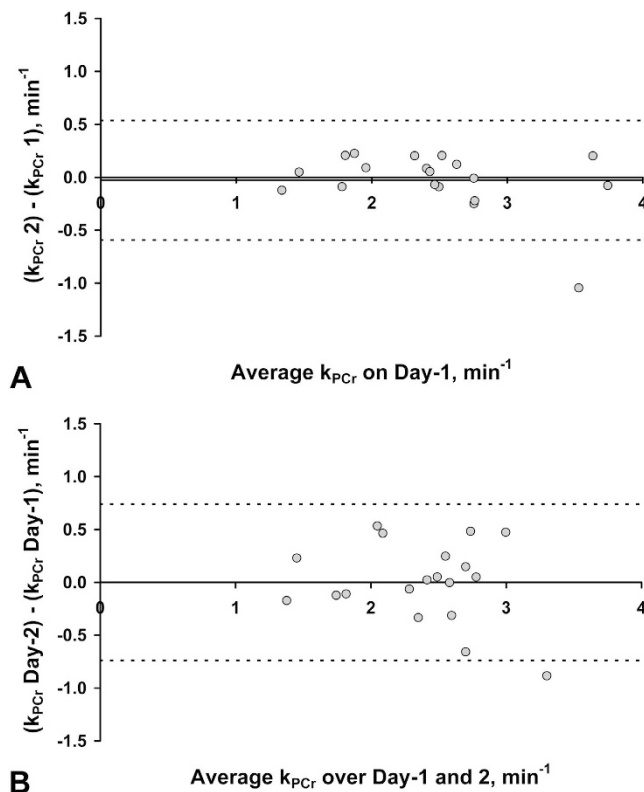


Figure 6. Bland-Altman plots for phosphocreatine recovery rate constant (k_{PCr}) test-retest measurements in 19 healthy volunteers. Bland-Altman analysis of k_{PCr} both within (A), and between (B), scan sessions. The plots show an insignificant mean bias (solid horizontal line) of -0.03 min^{-1} in (A) and 0.00 min^{-1} in (B), and 95% limits of agreement (dashed horizontal lines) of $-0.592; 0.537 \text{ min}^{-1}$ and $-0.739; 0.740 \text{ min}^{-1}$, in (A) and (B) respectively.

were 1.58 min^{-1} and 1.66 min^{-1} for recovery 1 and 2 respectively. No significant acidification occurred after either exercise, with the pH at end exercise rising from 7.01 at basal to 7.07 (both bout 1 and 2).

Discussion

We have described a novel and remarkably simple exercise design that allows efficient measurements of *in vivo* mitochondrial function in both healthy subjects and patients. This has been facilitated by exploiting the high density of the MR-compatible substance barium sulfate to apply load direct to the ankle, obviating the need for expensive and/or complex MR-compatible resistance or pulley equipment. The method produces well-controlled PCr depletion with patient compliance and permits highly reproducible measurements of post-exercise PCr recovery kinetics both within and between scan sessions, with coefficients of variation (5 and 8% respectively) that are comparable to the lowest reported values^{29–33} despite the fairly low PCr depletion in our study.

All exercise systems require a method to standardise PCr depletion between individuals and here we have done this using a measure of the volunteers' maximal voluntary contraction assessed by a dynamometer chair, although alternative methods could be used such as a fraction of lean body mass³⁴. The, on average, low fractional PCr depletion, and intersubject coefficient of variation of 30%, meant that the maximum percentage PCr depletion in visit 1 was only 33% (Fig. 5), thus the exercise was of sufficiently low intensity and duration to not yield significant acidification, which is known to slow PCr recovery⁵. This is important when using the PCr rate constant as a measure of mitochondrial function⁵, and may, in part, explain our high reproducibility values. Our ability to accurately measure the PCr kinetics post exercise at small PCr depletions is significantly aided by our high quality data (small PCr linewidths and small subcutaneous fat thicknesses in these volunteers), thus a target PCr depletion $>20\%$ may be advised in other cohorts and/or with other MR surface coils or acquisition techniques, at a field strength of 3 T.

One advantage of our exercise method is its easy-to-implement design that is readily translatable across sites and scanner models without mechanical alterations. The design does not require the participant to be strapped down to the scanner table and unlike most other procedures for exercising the quadriceps muscle *in situ*^{7,18,20,35} it permits the volunteer to be in the supine position which is important for patient comfort; this, together with the short exercise duration, ensures the exercise is easily tolerated. The dynamic nature of the exercise makes it suitable for patients with cardiovascular disease where forceful isometric exercise is not always recommended^{36,37}, and the set ankle weight circumvents the need to adjust exercise intensity by interpreting force feedback which can be challenging and particularly unsuitable for those with reduced mental capacity. The apparatus' high portability

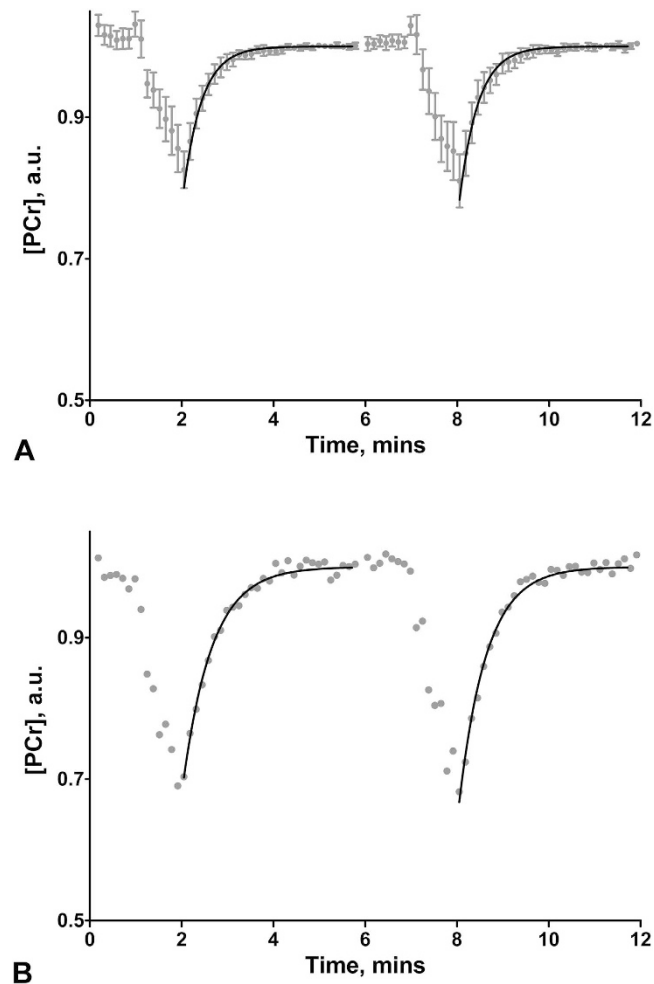


Figure 7. Phosphocreatine (PCr) timecourse in 19 healthy volunteers and in a lipodystrophic patient performing the optimised exercise protocol for measurement of PCr resynthesis rate post exercise. Data acquired on a Siemens MAGNETOM 3T Verio (Erlangen, Germany) in (A) 19 healthy volunteers and (B) a lipodystrophic patient performing the optimised exercise protocol of 1 min of rest, 1 min of exercise, followed by 4 minutes of rest, which is then all repeated. Grey circles represent [PCr] (mean [PCr] \pm 95% confidence interval of the mean in (A)), determined from ^{31}P -MRS spectra with a TR of 2 s, that have been quantified and then averaged to an effective TR of 8 s for clarity in this figure. In (A) participants [PCr] was normalised to their fully recovered post exercise PCr values (post exercise 8 s averaged time points 155–219 s inclusive), to permit intersubject comparison. The solid line represents the mono-exponential fit of the (mean in (A)) recovery rate constant to the PCr resynthesis data post exercise bouts one and two, with corresponding rate constants (k_{PCr}) $2.47 \pm 0.17 \text{ min}^{-1}$ and $2.44 \pm 0.15 \text{ min}^{-1}$ respectively in (A), and 1.58 min^{-1} and 1.66 min^{-1} respectively in the lipodystrophic patient (B).

permits straightforward pre-scanning rehearsal, which could make it effective for familiarisation in cohorts with, for example, learning difficulties. These factors adapt to the needs of the participant thereby aiding compliance and making this approach particularly well suited to clinical applications.

The cost, complexity and physical demands of specialised MR-compatible ergometers appears to be limiting the wider application of ^{31}P -MRS in clinical research. While detailed studies of muscle response to exercise, particularly at high intensities, requires sophisticated equipment, the assessment of PCr recovery kinetics is much less demanding and only requires a simple method to deplete the PCr pool. Our exercise design is superior to previously reported simple exercise designs³⁵ in that it easily permits an individual-specific workload by altering the ankle weight, does not place participants in an uncomfortable prone position, provides a more uniform workload over displacement, and is even easier to implement. The extremely simple method we have described here provides an inexpensive, patient-focused exercise design that is highly effective and suitable for frail participants or those with reduced mental capacity, offering the opportunity to implement measurements of muscle mitochondrial function more widely in a variety of clinical trial contexts.

References

- Sleigh, A. *et al.* Mitochondrial dysfunction in patients with primary congenital insulin resistance. *J Clin Invest* **121**, 2457–2461 (2011).
- Schon, E. A. & Manfredi, G. Neuronal degeneration and mitochondrial dysfunction. *J Clin Invest* **111**, 303–312 (2003).
- Bratic, A. & Larsson, N. G. The role of mitochondria in aging. *J Clin Invest* **123**, 951–957 (2013).
- Yu, E., Mercer, J. & Bennett, M. Mitochondria in vascular disease. *Cardiovasc Res* **95**, 173–182 (2012).
- Kemp, G. J., Ahmad, R. E., Nicolay, K. & Prompers, J. J. Quantification of skeletal muscle mitochondrial function by 31P magnetic resonance spectroscopy techniques: a quantitative review. *Acta Physiol* **213**, 107–144 (2015).
- Isbell, D. C. *et al.* Calf muscle perfusion at peak exercise in peripheral arterial disease: measurement by first-pass contrast-enhanced magnetic resonance imaging. *J Magn Reson Imaging* **25**, 1013–1020 (2007).
- Valkovic, L. *et al.* Interrelation of 31P-MRS metabolism measurements in resting and exercised quadriceps muscle of overweight-to-obese sedentary individuals. *NMR Biomed* **26**, 1714–1722 (2013).
- Valkovic, L. *et al.* Depth-resolved surface coil MRS (DRESS)-localized dynamic 31P-MRS of the exercising human gastrocnemius muscle at 7 T. *NMR Biomed* **27**, 1346–1352 (2014).
- Quistorff, B., Nielsen, S., Thomsen, C., Jensen, K. E. & Henriksen, O. A simple calf muscle ergometer for use in a standard whole-body MR scanner. *Magn Reson Med* **13**, 444–449 (1990).
- Wilson, J. R., McCully, K. K., Mancini, D. M., Boden, B. & Chance, B. Relationship of muscular fatigue to pH and diprotonated Pi in humans: a 31P-NMR study. *J Appl Physiol* **64**, 2333–2339 (1988).
- Gonzalez de Suso, J. M. *et al.* Development and characterization of an ergometer to study the bioenergetics of the human quadriceps muscle by 31P NMR spectroscopy inside a standard MR scanner. *Magn Reson Med* **29**, 575–581 (1993).
- Rodenburg, J. B., de Boer, R. W., Jeneson, J. A., van Echteld, C. J. & Bar, P. R. 31P-MRS and simultaneous quantification of dynamic human quadriceps exercise in a whole body MR scanner. *J Appl Physiol* **77**, 1021–1029 (1994).
- Ryschon, T. W. *et al.* A multimode dynamometer for *in vivo* MRS studies of human skeletal muscle. *J Appl Physiol* **79**, 2139–2147 (1995).
- Kemp, G. J. *et al.* Mitochondrial function and oxygen supply in normal and in chronically ischemic muscle: a combined 31P magnetic resonance spectroscopy and near infrared spectroscopy study *in vivo*. *J Vasc Surg* **34**, 1103–1110 (2001).
- Raymer, G. H., Marsh, G. D., Kowalchuk, J. M. & Thompson, R. T. Metabolic effects of induced alkalosis during progressive forearm exercise to fatigue. *J Appl Physiol* **96**, 2050–2056 (2004).
- Meyerspeer, M., Krssak, M., Kemp, G. J., Roden, M. & Moser, E. Dynamic interleaved 1H/31P STEAM MRS at 3 Tesla using a pneumatic force-controlled plantar flexion exercise rig. *MAGMA* **18**, 257–262 (2005).
- Raymer, G. H., Allman, B. L., Rice, C. L., Marsh, G. D. & Thompson, R. T. Characteristics of a MR-compatible ankle exercise ergometer for a 3.0 T head-only MR scanner. *Med Eng Phys* **28**, 489–494 (2006).
- Trenell, M. I., Sue, C. M., Kemp, G. J., Sachinwalla, T. & Thompson, C. H. Aerobic exercise and muscle metabolism in patients with mitochondrial myopathy. *Muscle Nerve* **33**, 524–531 (2006).
- Schrauwen-Hinderling, V. B. *et al.* Impaired *in vivo* mitochondrial function but similar intramyocellular lipid content in patients with type 2 diabetes mellitus and BMI-matched control subjects. *Diabetologia* **50**, 113–120 (2007).
- Layec, G. *et al.* Accurate work-rate measurements during *in vivo* MRS studies of exercising human quadriceps. *MAGMA* **21**, 227–235 (2008).
- Jenerson, J. A., Schmitz, J. P., Hilbers, P. A. & Nicolay, K. An MR-compatible bicycle ergometer for in-magnet whole-body human exercise testing. *Magn Reson Med* **63**, 257–261 (2010).
- Hosseini Ghomi, R., Bredella, M. A., Thomas, B. J., Miller, K. K. & Torriani, M. Modular MR-compatible lower leg exercise device for whole-body scanners. *Skeletal Radiol* **40**, 1349–1354 (2011).
- Sinha, S., Shin, D. D., Hodgson, J. A., Kinugasa, R. & Edgerton, V. R. Computer-controlled, MR-compatible foot-pedal device to study dynamics of the muscle tendon complex under isometric, concentric, and eccentric contractions. *J Magn Reson Imaging* **36**, 498–504 (2012).
- Tschiesche, K. *et al.* MR-compatible pedal ergometer for reproducible exercising of the human calf muscle. *Med Eng Phys* **36**, 933–937 (2014).
- Haynes, W. M. *CRC Handbook of Chemistry and Physics, 96th Edition.* (2015–2016) Available at: www.hbcpnetbase.com (Accessed: 16/11/2015).
- Phillips, A. C. *et al.* Defective mitochondrial function *in vivo* in skeletal muscle in adults with Down's syndrome: a 31P-MRS study. *PLoS One* **8**, e84031 (2013).
- Arnold, D. L., Matthews, P. M. & Radda, G. K. Metabolic recovery after exercise and the assessment of mitochondrial function *in vivo* in human skeletal muscle by means of 31P NMR. *Magn Reson Med* **1**, 307–315 (1984).
- Thankamony, A. *et al.* Low circulating levels of IGF-1 in healthy adults are associated with reduced beta-cell function, increased intramyocellular lipid, and enhanced fat utilization during fasting. *J Clin Endocrinol Metab* **99**, 2198–2207 (2014).
- McCully, K. K., Turner, T. N., Langley, J. & Zhao, Q. The reproducibility of measurements of intramuscular magnesium concentrations and muscle oxidative capacity using 31P MRS. *Dyn Med* **8**, 5 (2009).
- Layec, G. *et al.* Reproducibility assessment of metabolic variables characterizing muscle energetics *in vivo*: A 31P-MRS study. *Magn Reson Med* **62**, 840–854 (2009).
- Larson-Meyer, D. E., Newcomer, B. R., Hunter, G. R., Hetherington, H. P. & Weinsier, R. L. 31P MRS measurement of mitochondrial function in skeletal muscle: reliability, force-level sensitivity and relation to whole body maximal oxygen uptake. *NMR Biomed* **13**, 14–27 (2000).
- Edwards, L. M. *et al.* The reproducibility of 31-phosphorus MRS measures of muscle energetics at 3 Tesla in trained men. *PLoS One* **7**, e37237 (2012).
- van den Broek, N. M., De Feyter, H. M., de Graaf, L., Nicolay, K. & Prompers, J. J. Intersubject differences in the effect of acidosis on phosphocreatine recovery kinetics in muscle after exercise are due to differences in proton efflux rates. *Am J Physiol Cell Physiol* **293**, C228–237 (2007).
- Kemp, G. J. *et al.* Quantitative analysis by 31P magnetic resonance spectroscopy of abnormal mitochondrial oxidation in skeletal muscle during recovery from exercise. *NMR Biomed* **6**, 302–310 (1993).
- Whipp, B. J. *et al.* Simultaneous determination of muscle 31P and O₂ uptake kinetics during whole body NMR spectroscopy. *J Appl Physiol* **86**, 742–747 (1999).
- Lavie, C. J., Milani, R. V., Marks, P. & de Gruiter, H. Exercise and the heart: risks, benefits, and recommendations for providing exercise prescriptions. *Ochsner J* **3**, 207–213 (2001).
- Fletcher, G. F. *et al.* Statement on exercise: benefits and recommendations for physical activity programs for all Americans. A statement for health professionals by the Committee on Exercise and Cardiac Rehabilitation of the Council on Clinical Cardiology, American Heart Association. *Circulation* **94**, 857–862 (1996).

Acknowledgements

We are grateful to all the participants. This work was funded by the Clinical Research Infrastructure Grant. We thank the National Institute for Health Research (NIHR) Cambridge BioResource and S. Nutland, for facilitating

the recruitment of the 24 BioResource volunteers. We thank the NIHR Cambridge Biomedical Research Centre for funding the BioResource and we also acknowledge research grants from Addenbrooke's Charitable Trust and the British Society for Pediatric Endocrinology and Diabetes. D.B.S. is supported by the Wellcome Trust [091551] and the U.K. National Institute for Health Research (NIHR) Cambridge Biomedical Research Centre. A.S. and the Siemens MAGNETOM 3 T Verio scanner are funded by the NIHR via an award to the Cambridge NIHR/Wellcome Trust Clinical Research Facility. A.T. and D.B.D. are supported by the U.K. NIHR Cambridge Biomedical Research Centre. The funders had no role in study design, data collection and analysis, decision to publish, or preparation of the manuscript.

Author Contributions

A.S. conceived the experiment and analysed the data. A.S., V.L., A.T. and D.B.S. conducted the experiments. A.S., V.L., D.B.D., D.B.S. and T.A.C. contributed materials and tools. A.S. and G.J.K. wrote the manuscript, which was then reviewed by all authors.

Additional Information

Competing financial interests: The authors declare no competing financial interests.

How to cite this article: Sleight, A. *et al.* Simple and effective exercise design for assessing *in vivo* mitochondrial function in clinical applications using ^{31}P magnetic resonance spectroscopy. *Sci. Rep.* **6**, 19057; doi: 10.1038/srep19057 (2016).



This work is licensed under a Creative Commons Attribution 4.0 International License. The images or other third party material in this article are included in the article's Creative Commons license, unless indicated otherwise in the credit line; if the material is not included under the Creative Commons license, users will need to obtain permission from the license holder to reproduce the material. To view a copy of this license, visit <http://creativecommons.org/licenses/by/4.0/>