



Erratum

In the paper 'Validation of bio-impedance spectroscopy: effects of degree of obesity and ways of calculating volumes from measured resistance

values' by PL Cox-Reijven and PB Soeters, *Int J Obes* 2000; 24: 271–280, Figures 2 and 3 were incorrect. The correct figures are shown below.

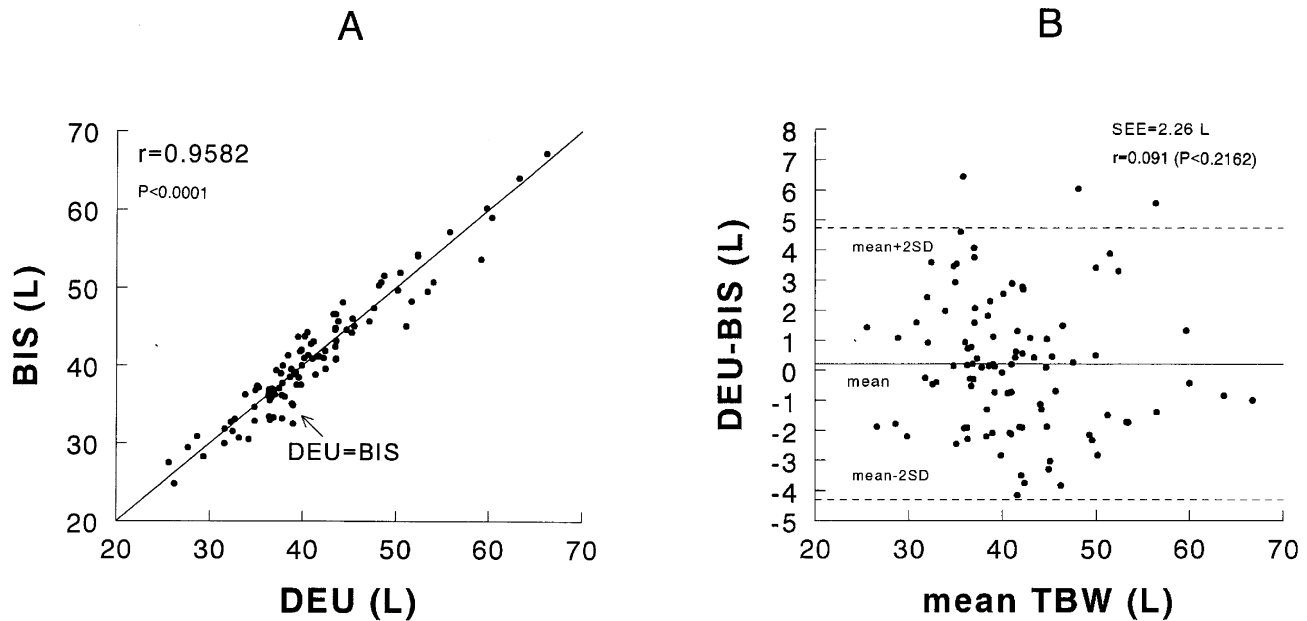


Figure 2 Comparison of total body water (TBW) measured with deuterium dilution (DEU) and bioelectrical impedance spectroscopy (BIS) in the total population. (A) The correlation between the two methods. (B) The difference between the two methods against their mean value. The horizontal line indicates the mean difference (bias) and the dotted lines indicate the 95% limits of agreement. The mean difference was not significantly different from zero.

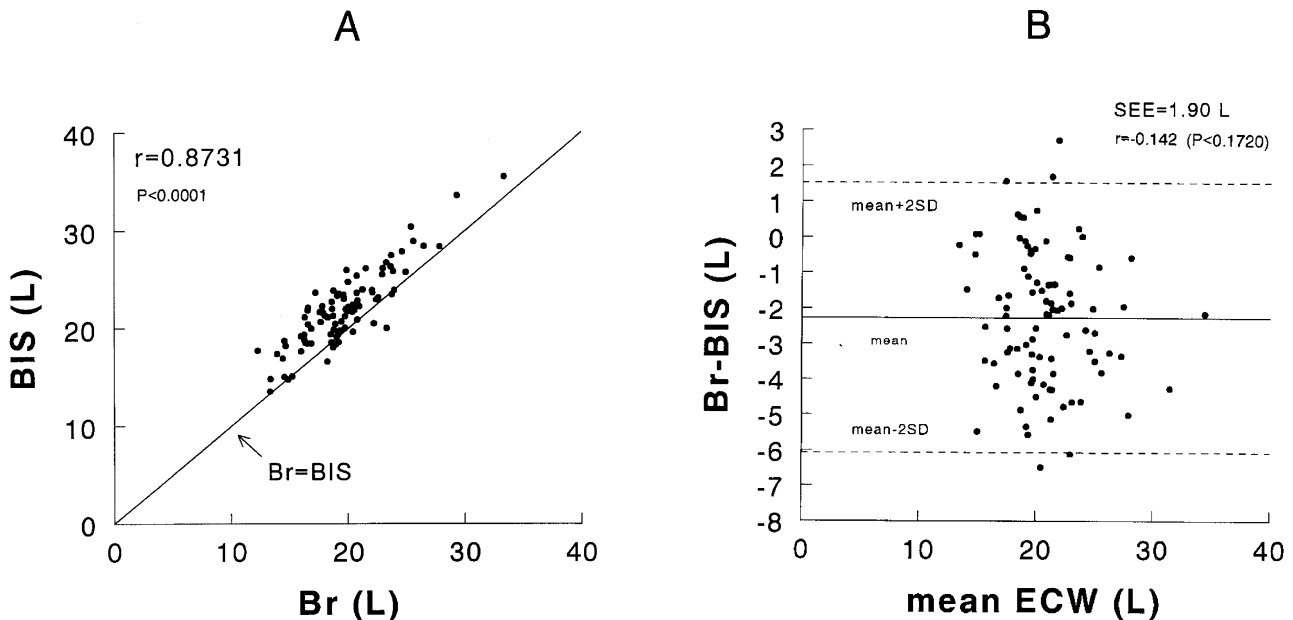


Figure 3 Comparison of extracellular water (ECW) measured with Br dilution (Br) and bioelectrical impedance spectroscopy (BIS) in the total population. (A) The correlation between the two methods. (B) The difference between the two methods against their mean value. The horizontal line indicates the mean difference (bias) and the dotted lines indicate the 95% limits of agreement. The mean difference was -2.27 (significantly different from zero, $P<0.005$).