



## Correction: Non-invasive measurement of sclerosis in cutaneous cGVHD patients with the handheld device Myoton: a cross-sectional study

Fuyao Chen · Laura E. Dellalana · Jocelyn S. Gandelman · Arved Vain · Madan H. Jagasia · Eric R. Tkaczyk

Published online: 17 January 2020  
© Springer Nature Limited 2020

**Correction to: Bone Marrow Transplantation**  
<https://doi.org/10.1038/s41409-018-0346-7>

In the original publication of this Correspondence, the y-axis was missing from Fig. 1a. The corrected figure is included in the HTML format and included with this correction.

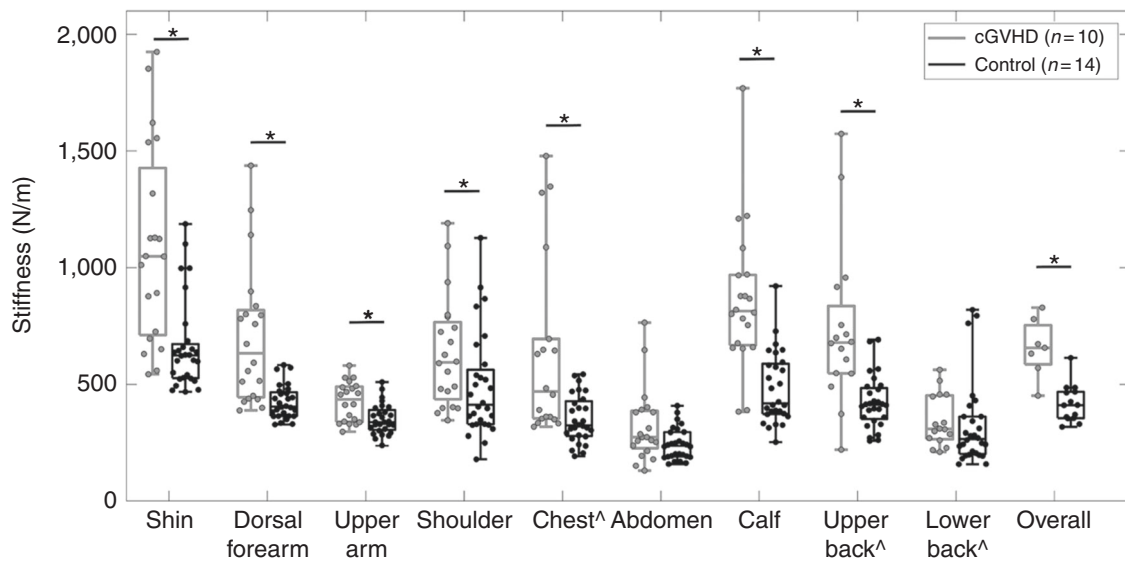


Fig. 1a